


USER'S MANUAL

Biogas Respirometer System (BRS)

- Biogas Respirometer / BMP Analyzer -

Model | BRS-110, BRS-200, BRS-800

Revision 10 January 2024

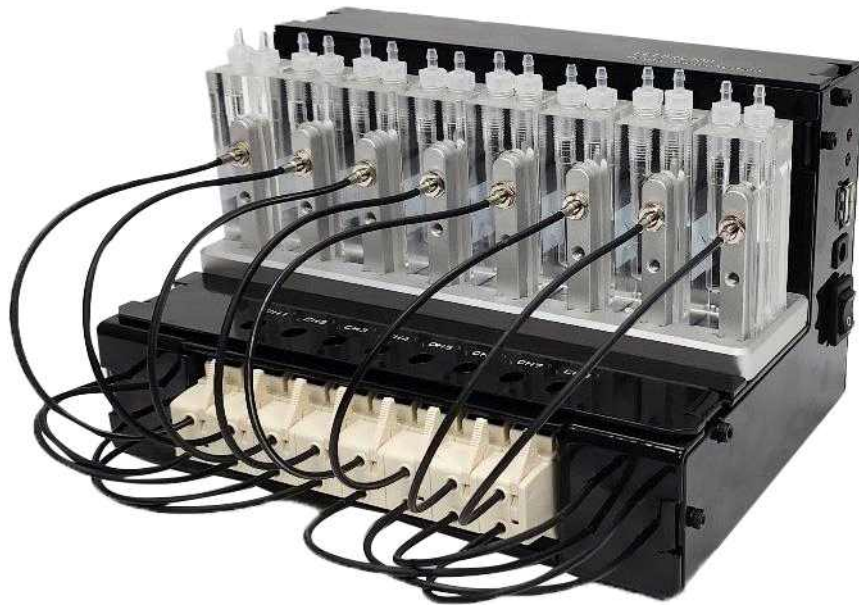

EET Eco-Environmental Technology Inc.

Don't discard the packaging box and silicon caps for plastic cells.
Save them if you need to return the product to the company for customer service

© 2011-2024. EET Inc. All Rights Reserved.

No part of this publication may be reproduced, transmitted, transcribed, stored in a retrieval system, or translated into any language or computer language, in any form, or by any means, electronic, mechanical, magnetic, optical, chemical, manual or otherwise, without the prior written permission of EET Inc.

Disclaimer

EET Inc. provides this document and the programs "as is" without warranty of any kind, either expressed or implied, including, but not limited to the implied warranties of merchantability or fitness for a particular purpose.

This document could contain technical inaccuracies or typographical errors. Changes are periodically made to the information herein; these changes will be incorporated in future revisions of this document. EET Inc. is under no obligation to notify any person of the changes.

CONTACT DETAILS

TEL	+82-33-243-6449
FAX	+82-33-242-6450
E-mail	eetech2011@daum.net
WEB	http://www.eetech.co.kr
Address for customer service	Room 101, Building No. 309, College of Agriculture and Life Science, Kangwon National University, Chuncheon-si, Gangwon State, South Korea Zip code : 24341

CONTENTS

Chapter I	Unboxing	
	Product lists (ordering information)	9
	How to check if the device works	10
	Program installation and operation flowchart	11
	Caution	12
Chapter II	BRS respirometer description	
	Principle of the respirometer	17
	Respirometer configuration	19
	BRS cells	23
	Select the measurement mode	24
	Connection of bioreactor and a BRS cell	26
Chapter III	BRS program	
	USB driver installation	31
	BRS Program installation and connection	32
	BRS program operation	34
	BRS program screen	38
Chapter IV	Troubleshooting and maintenance	
	How to calibrate the BRS cells for fixed bubble vol. mode	53
	Optic sensor adjustment	54
	Troubleshooting	56
	Disabling power saving mode	58
	Specifications	59

Chapter I

Unboxing

01

Product lists (ordering information)

▶ Product list for anaerobic respirometer

(BRS-110, BRS-200, and BRS-800)

- A main respirometer unit with four cells(BRS-110 and BRS-200) and eight cells(BRS-800) attached
- A USB cable and power adapter
- A sheet for factor values for each cell
- USB driver program, BRS program, and User's manual in an USB flash drive
- Syringe (10 mL), Needles (20G), Fittings, Tubing, Stir bars
- Wheaton serum bottles (500 mL), caps, and septa
- Internal CO₂ trap
- Special oil for the cells (50 mL), Cell oil needle
- External CO₂ trap unit (Optional)

※ The oil characteristics are different for BRS-110, BRS-200, and BRS-800, so the oils are not interchangeable.

▶ Products available

- Special oil for the cells (for BRS-110 ANR, BRS-200 ANR, and BRS-800 ANR), Cell oil needle
- Tubing, Fitting, Stir bars
- Serum bottles (125, 250, 500, and 1,000 mL), caps, and septa
- Internal CO₂ trap (BOD or BMP test)
- Water bath with stir plate (for 4 channels or 8 channels)
- BOD incubator with stir plate (for 4 channels or 8 channels)
- External CO₂ trap unit
- Metering valve
- O₂ gas regulator
- Syringes, Needles

02

How to check if the device works

- Carefully remove the device from the packaging box and connect the power cable to the right side of the device.
- Use your hand and press the BRS plastic cell down to prevent it from moving to remove the silicon caps from the plastic cells
- Keep the silicon caps and use them when sending the product to the headquarters for A/S.
- Insert the tubing supplied by the company directly into the left fitting (gas production) of the BRS cell for channel 1 to connect it.
- Turn on the power and slowly inject air through the tubing into the BRS cell using the syringe (5~10 mL) supplied by the company to create bubbles in the cell.
- Check if the two red LEDs on the optic sensors of channel 1 (right, left order) and the green LED on the right side of the device are blinking every time bubbles rise in the BRS cell (refer to the movie clip provided).
- Similarly, do the same things and check if the LEDs blink for channels 2, 3, and 4.
- If the LED does not blink, contact the company and refer to the manual to perform an optic sensor calibration (refer to the manual).
- If there is no problem, connect the device to the computer with the USB cable and install the BRS program.


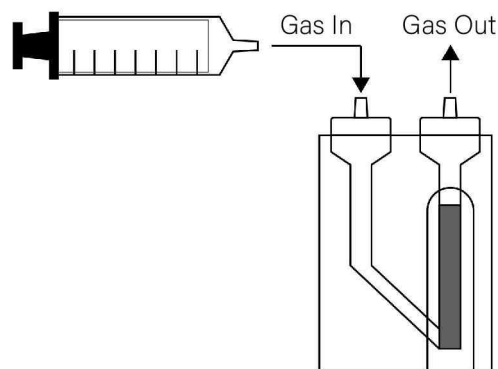


Fig. Connection with a syringe (5~10 mL) and the BRS cell

03


Program installation and operation flowchart

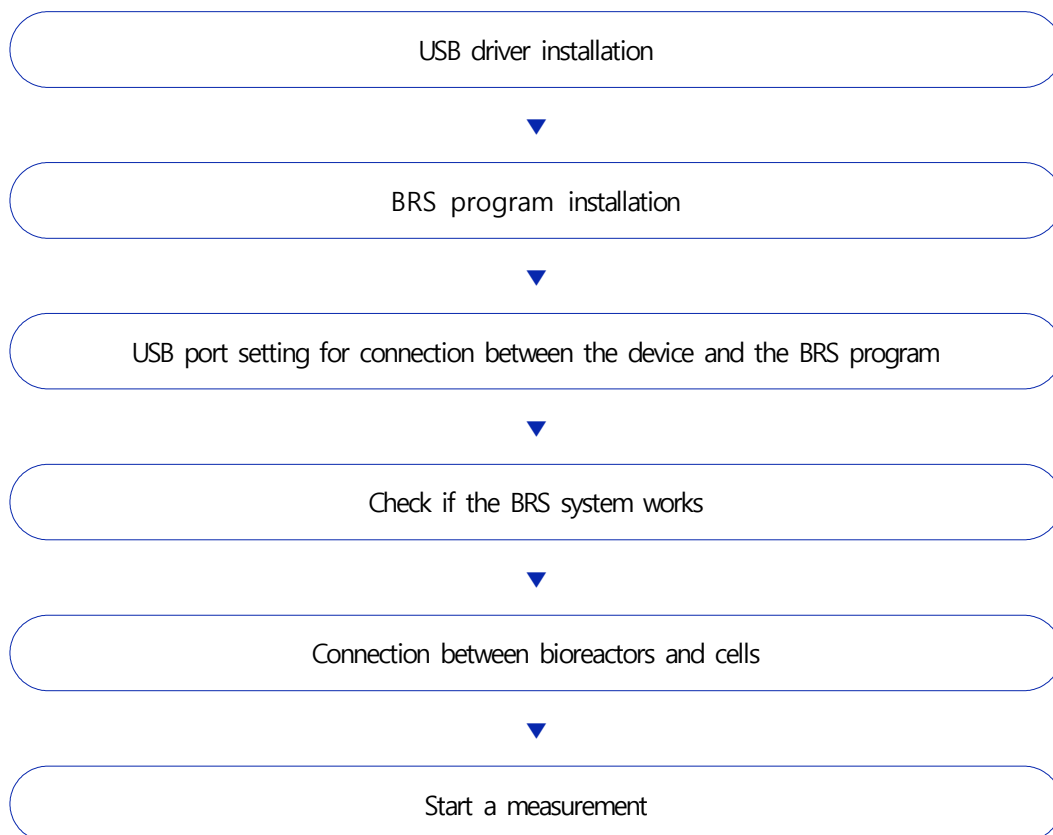


04

Caution


🔍 Device installation




Install the device horizontally.



Be careful not to drop the device.




Make sure the device does not come into direct contact with water.



Do not place the device near flammable materials.


Before measurement




You can connect up to four devices to one computer, and each port number must be set for each device. Also, make sure to turn off the power-saving mode of the computer.

[Factor]		
제곱	Factor 1	Factor 2
1	1.0000	0.0002
2	1.0005	0.0004
3	1.0010	0.0006
4	1.0015	0.0008


To obtain more accurate results, perform the experiment in a constant temperature chamber or incubator, while verifying that the factor values are accurately entered.




The BRS cells must be positioned exactly in the groove below. Do not switch the positions of the BRS cells.



Before starting the experiment, check if the BRS cells are filled with oil. After injecting air with a syringe into the BRS cell, the height of the oil level in the BRS cell should be higher than the H.sensor.




Make sure that the device's power or USB is properly connected. If the device's power or USB cable has been disconnected or if the port number of the option has been changed, be sure to restart the BRS program.




Before taking any measurements, confirm that when bubbles are generated using a syringe.


During measurement




Be careful as oil inside the BRS cell may flow out when the end of the syringe needle inserted to the septum of the bioreactor is blocked by water and pressure build up.



Do not move or shake the device.



Do not switch the cells.



If a raw data file or cumulative data file is open, measurement will not stop and data will not be saved. Therefore, be sure to close the file.

Chapter II

Respirometer Description

01

Principle of the respirometer

Theory

This product is a bubble-type microbial respiration measurement device that measures the amount and rate of gas generated (or consumed) in the reactor over time and displays it on graphs. The gas generated (or consumed) in the reactor rises in the form of bubbles in a BRS cell filled with oil and passes through two photo sensors located at the top and bottom of the BRS cell. The amount of gas generated (or consumed) over time can be measured in two modes 1) by counting the number of bubbles ([fixed bubble volume mode](#)) or 2) by measuring the bubble volume each time a bubble generated and adding these to calculate the total generated volume ([bubble volume calculation mode](#)).

BRS-110 and BRS-200 can be operated by fixed bubble volume mode and bubble volume calculation mode. BRS-800 can be operated by fixed bubble volume mode only.

[Fixed Bubble Volume Mode](#): Generally, as the airflow rate to the BRS cell increases from 0.3 mL/min to 20 mL/min, the bubble volume increases by about 20%. However, if the airflow rate is as small as 0.1 mL/min, that is, 144 mL/day, there is little differences in the volume of the generated bubbles, so the total volume is measured instead by counting the number of bubbles generated. This method is the fixed bubble volume mode.

[Bubble Volume Calculation Mode](#): Bubble volume is measured each time a bubble is created. The bubble volume is measured using two optic sensors, specifically a low and a high sensor, with a travel distance. T1 is the times taken by the bubble to cross the high sensor and T2 is the time elapsed from when a bubble first touches the lower sensor until it touches the upper sensor. Using T1 and T2 the volume of the bubble can be calibrated by adding different air flow rates using a syringe pump.

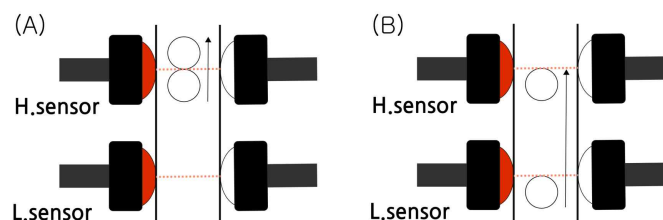


Fig. BRS cell depiction of (A) T1 and (B) T2

◉ Applications


- Biogas production
- BMP test
- Biochemical hydrogen potential
- Green energy studies
- Laboratory respiration studies
- Soil and compost respiration
- Respiration of plants/animals
- Measurement of oxygen consumption
- Oxygen uptake rate (OUR)
- Toxicity screening
- Biodegradation test
- Treatability assessment

02

Respirometer configuration

🔍 Respirometer


(BRS-110 and BRS-200)

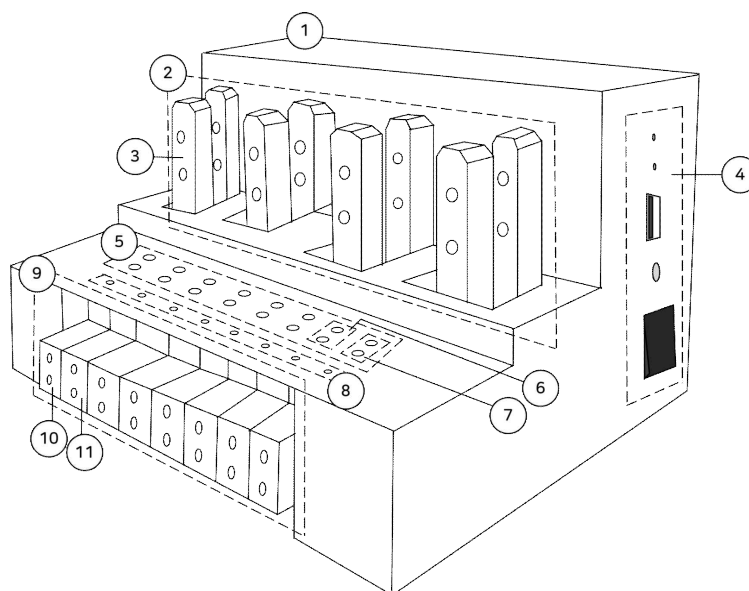

- | | | |
|-------------------------|---------------------------|--|
| ① Main board | ⑤ Optic sensor adjustment | ⑨ Optic sensors |
| ② BRS cells | ⑥ H.sensor adjustment | ⑩ Optic sensors for high position (H.sensor) |
| ③ Cell Support | ⑦ L.sensor adjustment | ⑪ Optic sensors for low position (L.sensor) |
| ④ Power and data output | ⑧ Red LEDs | |


▶ Respirometer

(BRS-800)

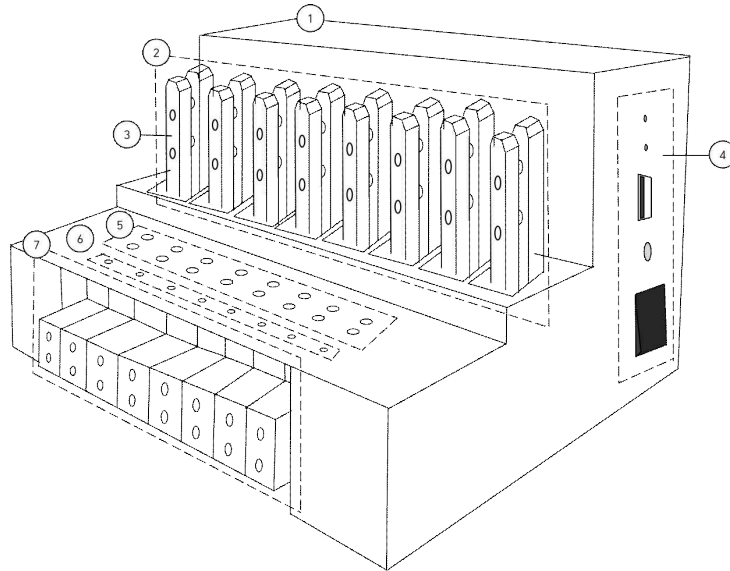

- ① Main board
- ② BRS cells
- ③ Cell Support
- ④ Power and data output
- ⑤ Optic sensor adjustment
- ⑥ Red LEDs
- ⑦ Optic sensors

▶ Power and data output

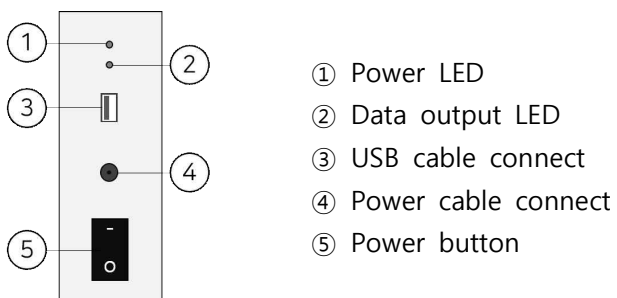


- ① Power LED
- ② Data output LED
- ③ USB cable connect
- ④ Power cable connect
- ⑤ Power button

Optic sensors


(BRS-110 and BRS-200)

<Parts for adjustment>

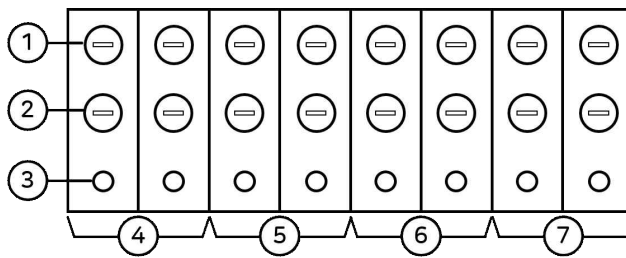


- ① Fine adjustment
- ② Coarse adjustment
- ③ Red LEDs
- ④ Ch.1
- ⑤ Ch.2
- ⑥ Ch.3
- ⑦ Ch.4

<Optic sensors>

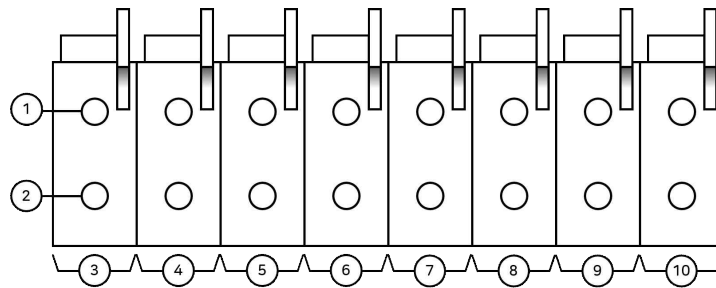

- | | | |
|-----------------|-----------------|-----------------|
| ① Light receive | ③ Ch.1 H.sensor | ⑦ Ch.3 H.sensor |
| ② Light send | ④ Ch.1 L.sensor | ⑧ Ch.3 L.sensor |
| | ⑤ Ch.2 H.sensor | ⑨ Ch.4 H.sensor |
| | ⑥ Ch.2 L.sensor | ⑩ Ch.4 L.sensor |

<Connection of optic cable to optic sensor>

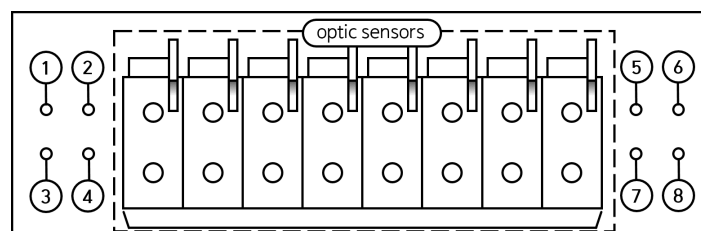


- | | |
|-----------------|-----------------|
| ① Ch.1 H.sensor | ⑤ Ch.3 H.sensor |
| ② Ch.2 H.sensor | ⑥ Ch.4 H.sensor |
| ③ Ch.1 L.sensor | ⑦ Ch.3 L.sensor |
| ④ Ch.2 L.sensor | ⑧ Ch.4 L.sensor |


Optic sensors

(BRS-800)

<Parts for adjustment>

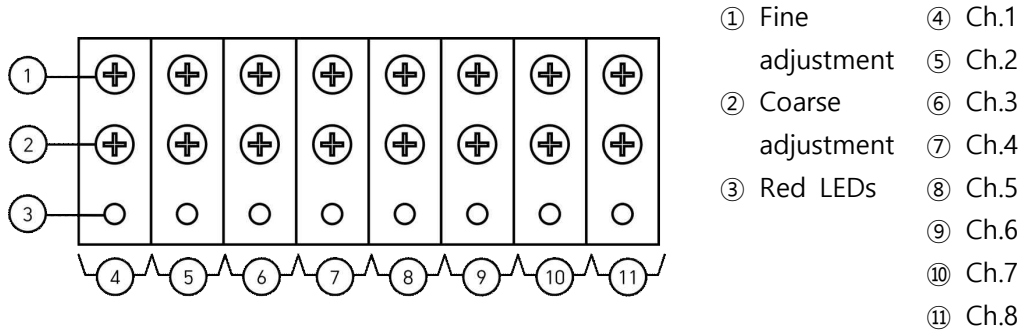


<Optic sensors>

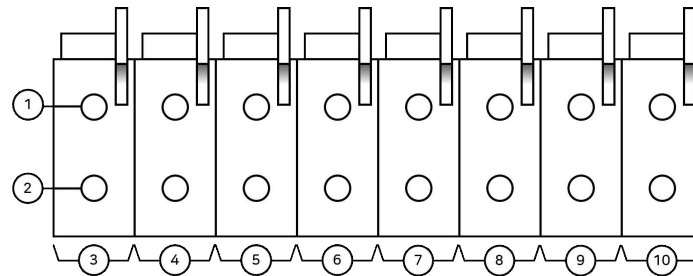

- | | | |
|-----------------|---------------|---------------|
| ① Light receive | ③ Ch.1 sensor | ⑦ Ch.5 sensor |
| ② Light send | ④ Ch.2 sensor | ⑧ Ch.6 sensor |
| | ⑤ Ch.3 sensor | ⑨ Ch.7 sensor |
| | ⑥ Ch.4 sensor | ⑩ Ch.8 sensor |

<Connection of optic cable to optic sensor>

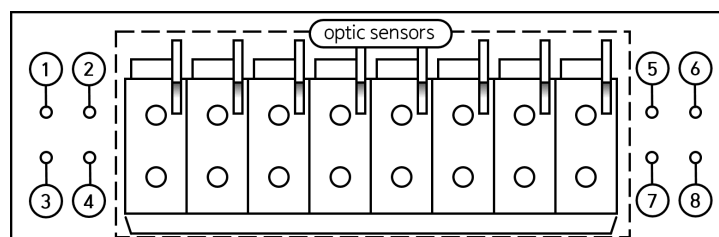

- | | |
|---------------|---------------|
| ① Ch.1 sensor | ⑤ Ch.5 sensor |
| ② Ch.2 sensor | ⑥ Ch.6 sensor |
| ③ Ch.3 sensor | ⑦ Ch.7 sensor |
| ④ Ch.4 sensor | ⑧ Ch.8 sensor |

◉ BRS cells

	Measurable flow rate	Oil volume
BRS-110	0~1 mL/min	2.2 mL
BRS-200	1~5 mL/min	12.0 mL
BRS-800	0~0.2 mL/min	1.6 mL

◉ Connection of a bioreactor and a BRS cell

- For measuring gas production from a bioreactor, the bioreactor should be connected to the left top fitting of a cell using tubing as shown in the below figure. The generated gas will push out the oil in a cell, and the gas turns into gas bubbles in the oil.

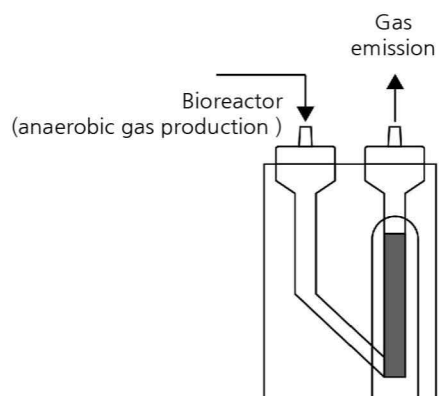


Fig. Connection of a bioreactor and a BRS cell for anaerobic gas production

04

Selection of the measurement mode

◉ Bubble vol. calculation mode

- Calculate volumes of bubbles every time bubbles are generated.
- Use when the gas generation rate is more than 0.1 mL/min.
- Input the factor values according to the temperature and the minimum/maximum reference bubble volume in the settings at the BRS program.
- BRS-110 and BRS-200 can use in this mode.

◉ Fixed bubble vol. mode

- When the gas generation rate is small (within 0.1 mL/min), there is little difference in bubble volumes. In this case, calculate the total amount of generation/consumption by fixing the bubble volume and multiplying by the number of bubbles.
- Enter the fixed bubble volume value according to the temperature in the settings at the BRS program.
- BRS-110, BRS-200, and BRS-800 can use in this mode.

	Bubble Volume Calculation Mode	Fixed Bubble Volume Mode
Definition	<ul style="list-style-type: none"> □ Calculate volumes of bubbles every time bubbles are generated. □ Bubble volume will increase as the gas flow rate increases to over 0.1 mL/min 	<ul style="list-style-type: none"> □ When the gas flow rate is less than 0.1 mL/min, bubble volumes are almost the same. The bubble volume can be fixed
Advantage	<ul style="list-style-type: none"> □ It is possible to measure the bubble volume every time a bubble is generated, so errors will be small 	<ul style="list-style-type: none"> □ Fixed bubble volume mode eliminates the need for periodic calibration.
Disadvantage	<ul style="list-style-type: none"> □ It is necessary to periodically inject a fixed amount of gas manually and determine whether the equipment needs calibration (F3 calibration is possible in the laboratory if necessary) 	<ul style="list-style-type: none"> □ To measure gas flow rate above 0.1 mL/min, the bubble vol. calc. mode should be used.

Mode
selection

□ Choose this mode when the gas flow rate is higher than 0.1 mL/min (the bubble generation rate is such that one bubble is generated and another bubble is generated within 1 to 5 seconds)

□ Choose this mode when the gas flow rate is lower than 0.1 mL/min (the bubble generation rate is such that one bubble is generated, and after waiting about 5 seconds or more, another bubble is generated)

05

Connection of a bioreactor and a BRS cell

🔍 Connection of bioreactor and a BRS cell

<Gas production>

- ① Install the BRS respirometer in an incubator set at the desired temperature.
- ② Place the medium and stir bars in the uninoculated bioreactors, and sparge for 5-10 minutes with N_2 gas to remove dissolved oxygen. Cover the reactors with sealed caps, each containing a septum.
- ③ Place the bioreactors in a water bath to adjust medium temperature to the desired experimental temperature quickly.
- ④ After the medium temperature of the bioreactors has increased, move them to the incubator and place them on a stirrer, then add microorganisms using a syringe with a needle.
- ⑤ When microorganisms are added, pressure is created in the headspace, so after adding the microorganisms, insert a needle into the septum to release the pressure; then, remove the needle after a few seconds.
- ⑥ To connect the bioreactors to the BRS cells, insert a needle connected at the end of the tubing into the septum as shown in the following figure.
- ⑦ Add N_2 gas (1~2 mL) to the reactor headspace through the septum using another syringe with a needle slowly and check for formation of bubbles in the cell. Confirm that data is being transmitted to the computer, and start measurement.

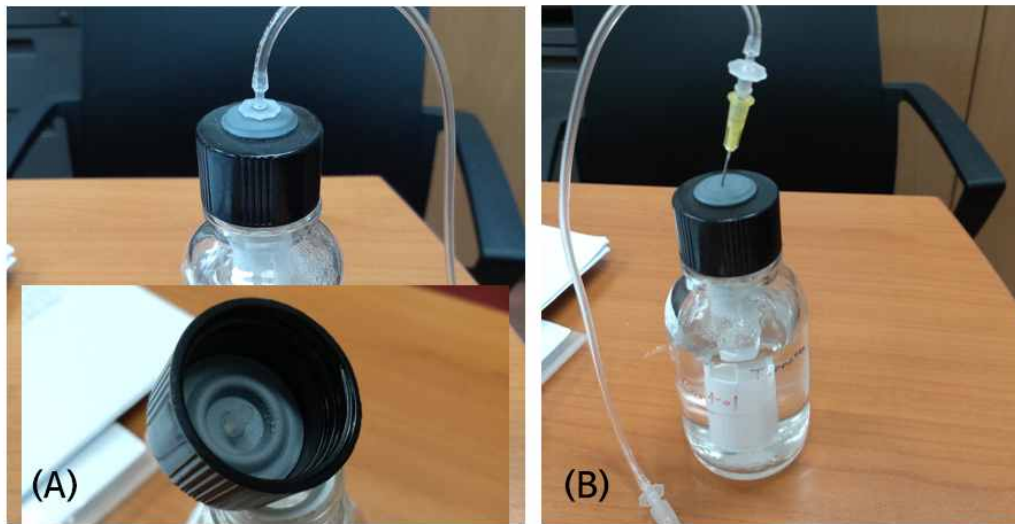


Fig. Examples of connection between bioreactor and tubing from a BRS cell using septum with fitting (A) and a needle (B)

Information for connecting of bioreactor and a cell

- ① It is important to use the same type of stir bar in each reactor and ensure that the stirring speed is uniform and sufficiently fast since the rate at which oxygen gas dissolves in the solution can vary depending on the stirring speed.
- ② When bubbles pass through the H.sensor and L.sensor, the LED (red) in the optical sensor blinks and the data is transmitted to the BRS program, checking that the LED (green) on the right side of the device is blinking.
- ③ The CO_2 generated by the biological reaction can be removed in the form of CO_3^{2-} through 5 M KOH (280.5 g KOH/L) in the CO_2 trap.

Chapter III

BRS program

01

USB driver installation

▶ USB driver installation

<Install only when connecting the device to the computer for the first time>

- ① Connect the USB cable to the device and the computer
- ② Unzip the separately attached CP210.zip
- ③ Open Device manager on control panel
- ④ Confirm that Silicon Labs CP210x CP2102 USB to UART Bridge Controller(hereinafter "CP210x") is created in the "Port (COM and LPT)" item
- ⑤ CP210x-(Right)-Click [Properties]
- ⑥ Click on Driver-Update Driver
- ⑦ Click Find Driver Software on your computer
- ⑧ After clicking [Browse], select the extracted folder, and then proceed to complete installation

▶ USB port setting and check

- ① Make sure that the BRS-110's power is on and that the USB cable is connected.
- ② Click [Port (COM and LPT)] in [Device Manager], and then click CP210x (COM1).
- ③ Set "bit 38400, data bit 8, no parity, stop bit 1, no flow control" in "port setting".
- ④ Click the "Advanced" button to check the COM port number.
- ⑤ Click the [OK] button to close the setting window

02

BRS program installation and connection

▶ BRS program installation

- ① Unzip the BRS setup file
- ② Click "BRS setup.exe" to install a program
- ③ Default installed folder is C:\WEETWBRSW
- ④ Be sure to turn off computer sleep mode after the installation is complete

▶ BRS program uninstall

- ① Close the BRS program
- ② If a Raw or Data file is open, the BRS program may not be properly uninstalled
- ③ Therefore, if any of these files are open, please close them before attempting to uninstall the BRS program
- ④ Uninstall the BRS program from Apps or click the unins000.exe file on C:\WEETWBRSW
- ⑤ Raw folder and Data folder are not deleted by uninstalling the program; if necessary manually delete the two folders with data

▶ Connection of a device and a program

- ① Launching the BRS program, click on Menu - Option - Option
- ② Activate the "Use" button according to the number of devices being used
- ③ Check the port number in the BRS port setting
- ④ Open the Device Manager to check the port number from Port(COM&LPT)
- ⑤ If the port number in the BRS program and port number in the Device Manager are different, adjust the port number in the Device Manager to match the BRS port number
- ⑥ Click the OK button to close and restart the BRS program

- ⑦ If the port number in the BRS program and port number in the Device Manager are the same, click the Cancel button to close the option window
- ⑧ The port numbers of all installed BRS programs must be different

03

BRS program operation

 BRS program operation

- ① Run the BRS program by clicking on the BRS shortcut on the desktop .
- ② To connect the respirometer and the BRS program, match the COM port number with the port number in the BRS port setting, and restart the BRS program.
- ③ If the connection fails even after restarting the BRS program, reboot the computer and then run the BRS program again.
- ④ Check the connection in the lower left corner of the program based on the yellow color of the figures ①~④.

 Settings

- ① Click on the menu "Settings"
- ② Choose the experiment mode (variable bubble vol. mode or fixed bubble vol. mode)
- ③ Enter the settings value provided by company
- ④ Input the actual operating temperature that the user is experimenting with, and change the Time interval, Save interval of cumulative data, or Save interval of raw data according to the user's convenience
- ⑤ If the provided values are not entered correctly, accurate measurement results may not be obtained. Make sure to enter them correctly

 Start measurement

- ① After clicking on the "Measurement" menu, check if channels 1 to 4 are all in waiting mode
- ② Select the channels to be measured and click the "Start measurement" button
- ③ Multiple channels can be started simultaneously
- ④ Confirm that the channels that started the measurement has changed to "Measuring" in the channel information

🕒 Check the data

To view cumulative data find the desired file in the corresponding data folder shown below and load it into an Excel program. The data is represented as shown in the figure below.

Data folder

<Location>

- BRS I : C:\WEET\BRS\BRS1\Data
- BRS II : C:\WEET\BRS\BRS2\Data
- BRS III : C:\WEET\BRS\BRS3\Data
- BRS IV : C:\WEET\BRS\BRS4\Data

<File name>

- BRS no_Data_Date_Time_No. of start
- ex) B1_Data_20221221_160000_1
- ex) B2_Data_20221221_170000_1

Start time	3/13/2023 16:26:22	3/13/2023 16:26:22	3/13/2023 16:26:22	3/13/2023 16:26:22
Product no	Test_BRS			
Test name	Test1	Test2	Test3	Test4
Factor1	2.1816	2.1284	2.0054	1.9241
Factor2	0.0092	0.0073	0.0025	0.0031
Factor3	1	1	1	1
Minutes	Ch 1	Ch 2	Ch 3	Ch 4
0	0	0	0	0
1	0.0897	0.0888	0.0897	0.0926
2	0.1794	0.1776	0.1794	0.1812
3	0.2995	0.2962	0.2983	0.3001

Fig. An example of data file in excel (BRS-110 and BRS-200)

Start time	3/13/2023 16:26:22	3/13/2023 16:26:22	3/13/2023 16:26:22	3/13/2023 16:26:22	3/13/2023 16:26:22	3/13/2023 16:26:22	3/13/2023 16:26:22	3/13/2023 16:26:22
Product no	Test_BRS							
Test name	Test1	Test2	Test3	Test4	Test5	Test6	Test7	Test8
Factor1	2.1816	2.1284	2.0054	1.9241	2.1816	2.1284	2.0054	1.9241
Factor2	0.0092	0.0073	0.0025	0.0031	0.0092	0.0073	0.0025	0.0031
Factor3	1	1	1	1	1	1	1	1
Minutes	Ch 1	Ch 2	Ch 3	Ch 4	Ch 5	Ch 6	Ch 7	Ch 8
0	0	0	0	0	0	0	0	0
1	0.0897	0.0888	0.0897	0.0926	0.0897	0.0888	0.0897	0.0926
2	0.1794	0.1776	0.1794	0.1812	0.1794	0.1776	0.1794	0.1812
3	0.2995	0.2962	0.2983	0.3001	0.2995	0.2962	0.2983	0.3001

Fig. An example of data file in excel (BRS-800)

<If a raw file or cumulative data file is open, automatic saving and stopping measurement may not be executed, so the opened file (raw file and/or cumulative data file) must be closed>

<If you need to check the data value during the experiment, press the small save button just next to "Save interval of cumulative data" or "Save interval of raw data" to update to the latest data. Then, copy the raw or data file you want to view, paste it into another folder, and open the file to check>

<When the "Start measurement" is clicked, a data and raw file will be created automatically in the folder>

Raw folder

<Location>

BRS I : C:\WEET\BRS\BRS1\Raw
 BRS II : C:\WEET\BRS\BRS2\Raw
 BRS III : C:\WEET\BRS\BRS3\Raw
 BRS IV : C:\WEET\BRS\BRS4\Raw

<File name>

BRS no._Raw Ch no._Date_Time_Test name
 ex) B1_Raw1_20221221_160000_Test1

ex) B2_Raw2_20221221_170000_N2

Time	T1	T2	Ch 1
3/13/2023 20:00	100.1	204.8	0.05
3/13/2023 20:14	100.9	203.9	0.05
3/13/2023 21:22	100.8	204.1	0.05
3/13/2023 21:25	100.5	204.6	0.05


Fig. An example of raw file in excel

▶ Data convert

- Time interval in the data file can be changed using raw files in the "Data convert" menu, for example, time interval 1 hour to 10 min interval.
 - In the "Data convert" menu, four raw files can be chosen by clicking files in the file list
 - After choosing files, change cumulative time (time interval) and click "Apply"
 - Then, data having changed time intervals can be obtained

Common information

(BRS-110, BRS-200, and BRS-800)

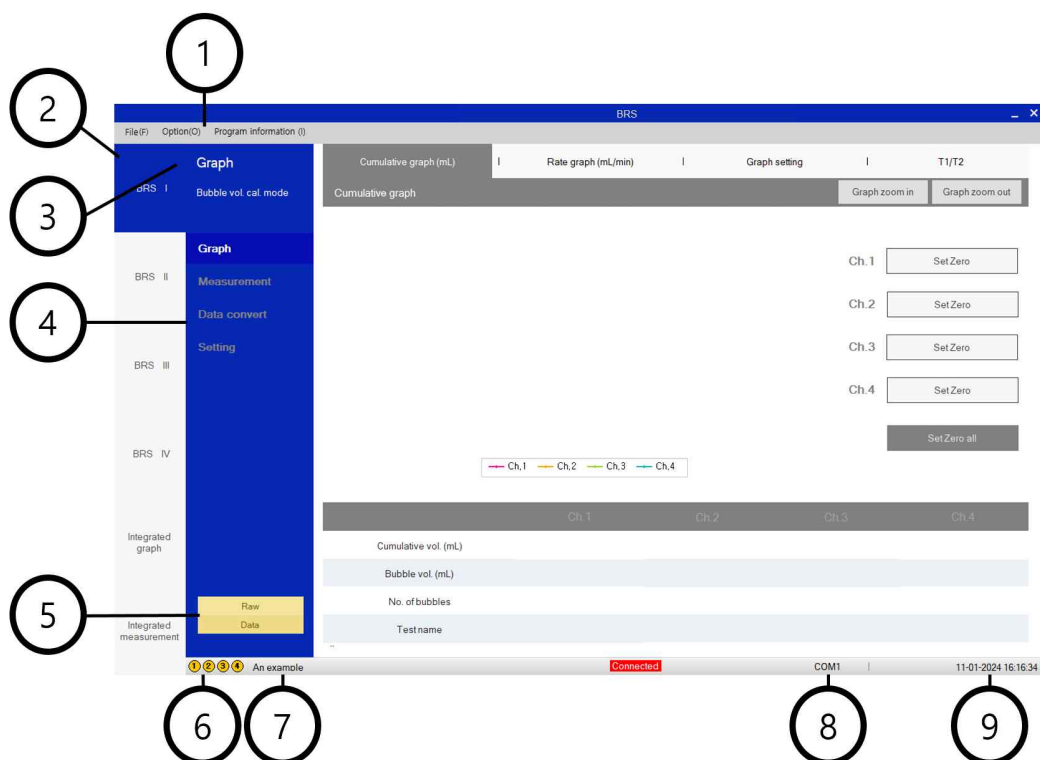

① Menu

- File (F) : Time calculator (Ctrl+T), Exit (Alt+X)
- Option (O) : Option (Ctrl+O), Device manager (Ctrl+D),
- Program information (I) : Product no. registration (Ctrl+R), Update list (Ctrl+U), Program information (Ctrl+I)

② BRS selection

- This program can control 4 BRS respirometers simultaneously

③ Sub-menu and current operation mode

- Check the bubble vol. calc. mode or fixed bubble vol. mode(BRS-110 and

BRS-200)

- Fixed bubble vol. mode is fixed in BRS-800

④ Menu

- Graph, Measurement, Data convert, Setting

⑤ Button for opening Raw folder or Data folder

⑥ Device connection status


- Measuring (green), Waiting (yellow), Disconnected (black)

⑦ Product no.

⑧ Port no.

⑨ Date and time

▶ Graph
[<Graph>](#)

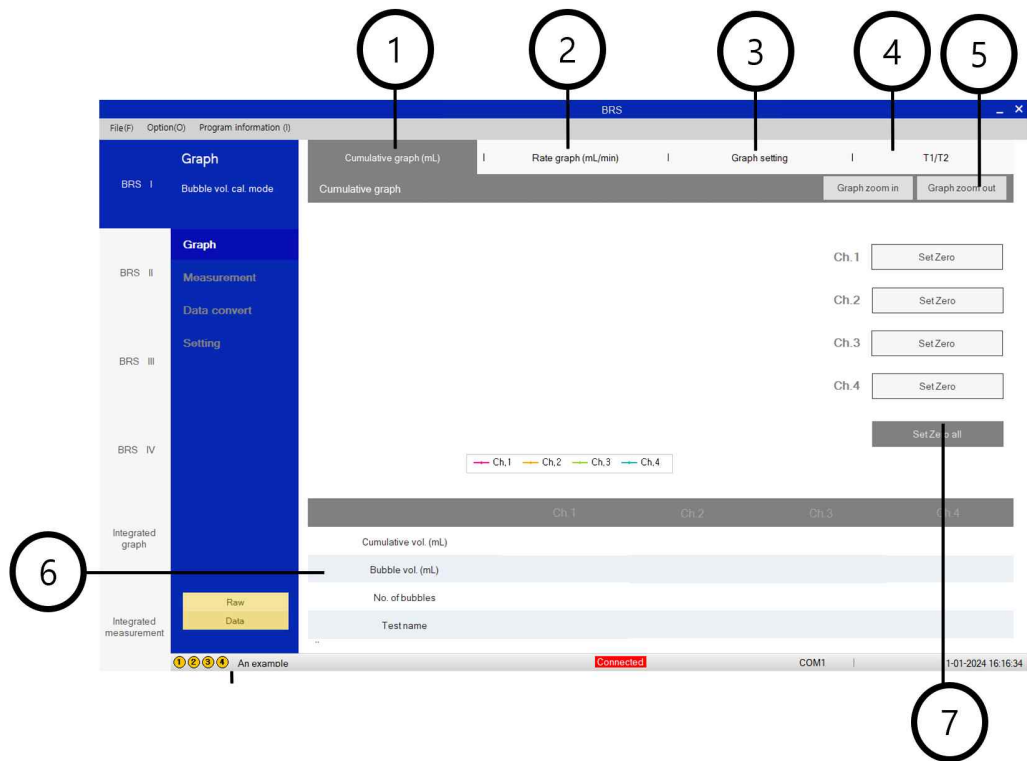


① Cumulative graph

② Rate graph

- ③ Graph setting
- ④ T1, T2
- ⑤ Zoom in and zoom out of graph
- ⑥ Data table
- ⑦ Buttons for semi-continuous operation


[<Graph setting>](#)

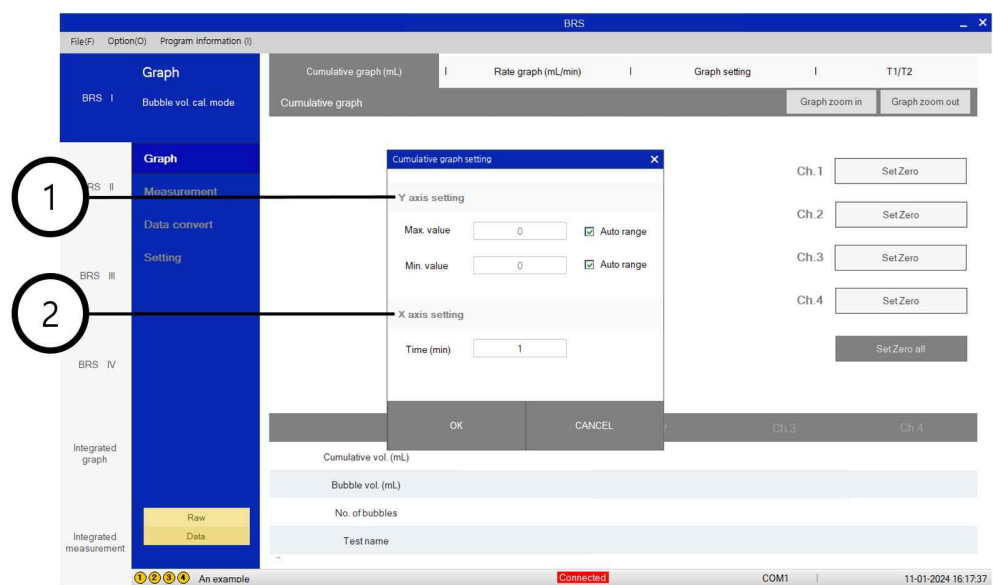

- ① Y axis setting
 - Max. and min. values for Y axis
- ② X axis setting
 - Time interval for zoom in and zoom out

Measurement

(BRS-110 and BRS-200)

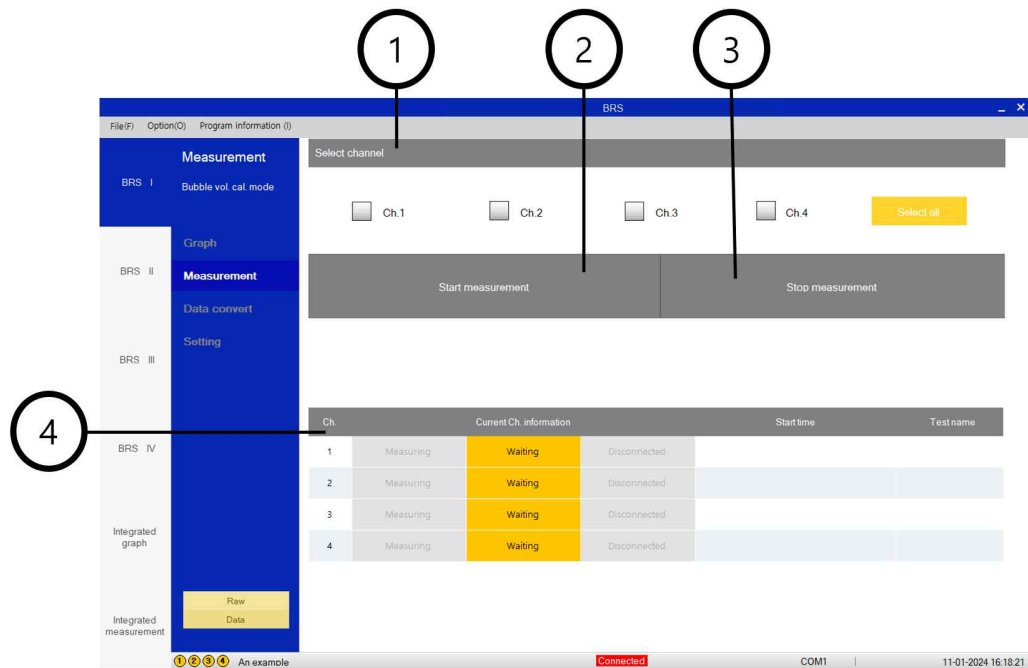

① Select channel

- Select each channel to start or stop
- By clicking Select all button, all channels are selected to start or stop measurement


② Start measurement

③ Stop measurement

④ Current status

- It is possible to check the current status, measurement start time, and experiment name for each channel
- Measuring (green), Waiting (yellow), Disconnected (black)

(BRS-800)

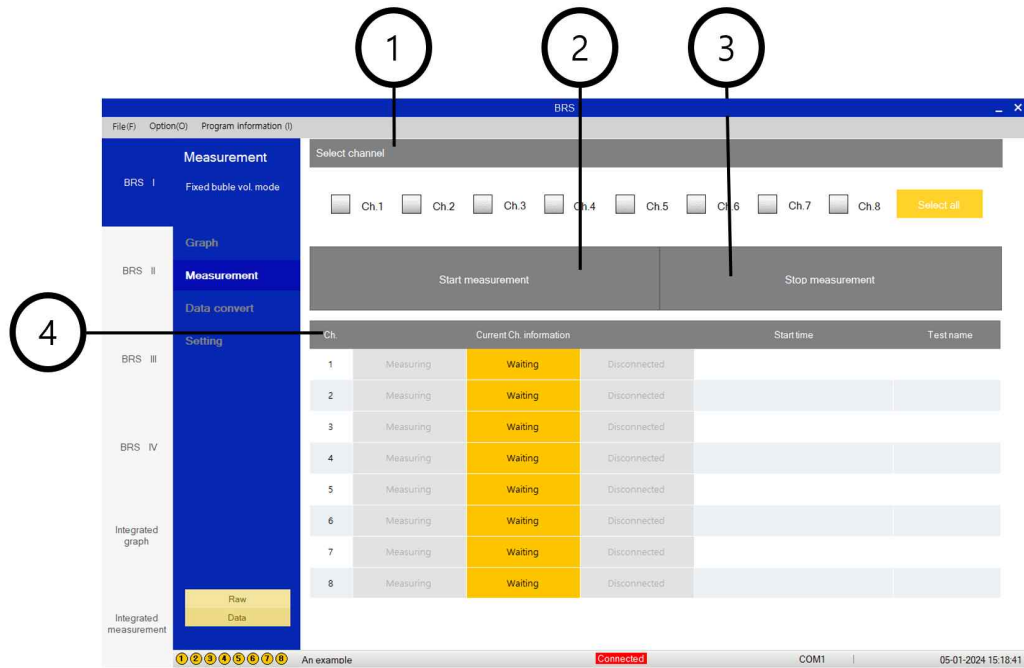

① Select channel

- Select each channel to start or stop
- By clicking Select all button, all channels are selected to start or stop measurement


② Start measurement

③ Stop measurement

④ Current status

- It is possible to check the current status, measurement start time, and experiment name for each channel
- Measuring (green), Waiting (yellow), Disconnected (black)

Data convert

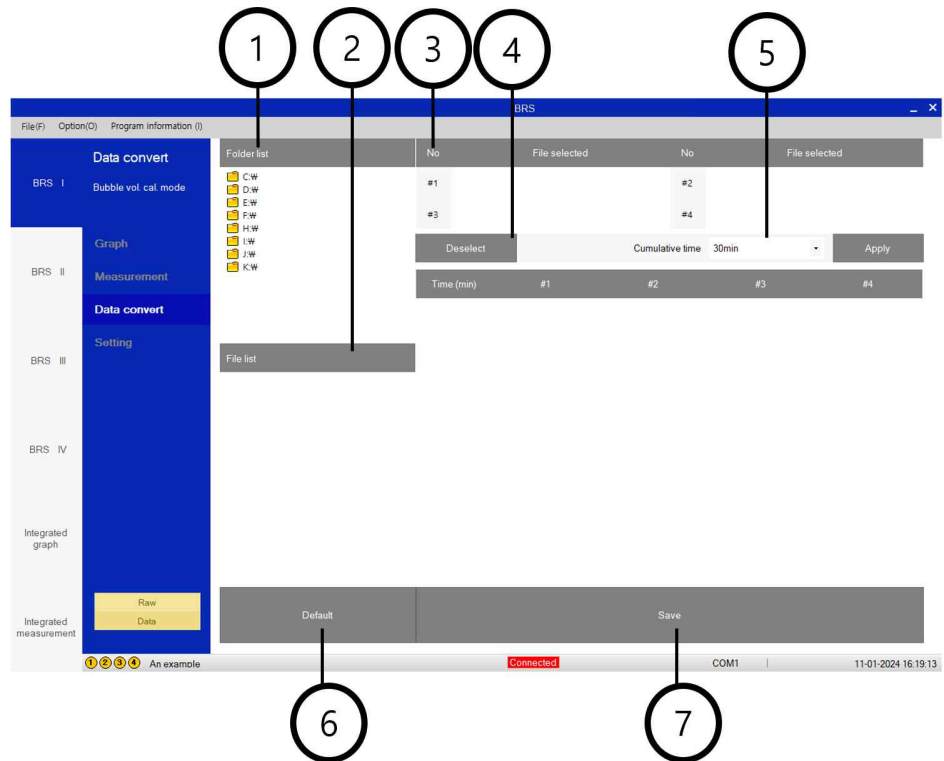


- ① Folder list
- ② File list
- ③ Selected file
- ④ Deselect
- ⑤ Cumulative time
- ⑥ Reset
- ⑦ Save converted file

Setting


(BRS-110 and BRS-200)

<Bubble vol. calc. mode>

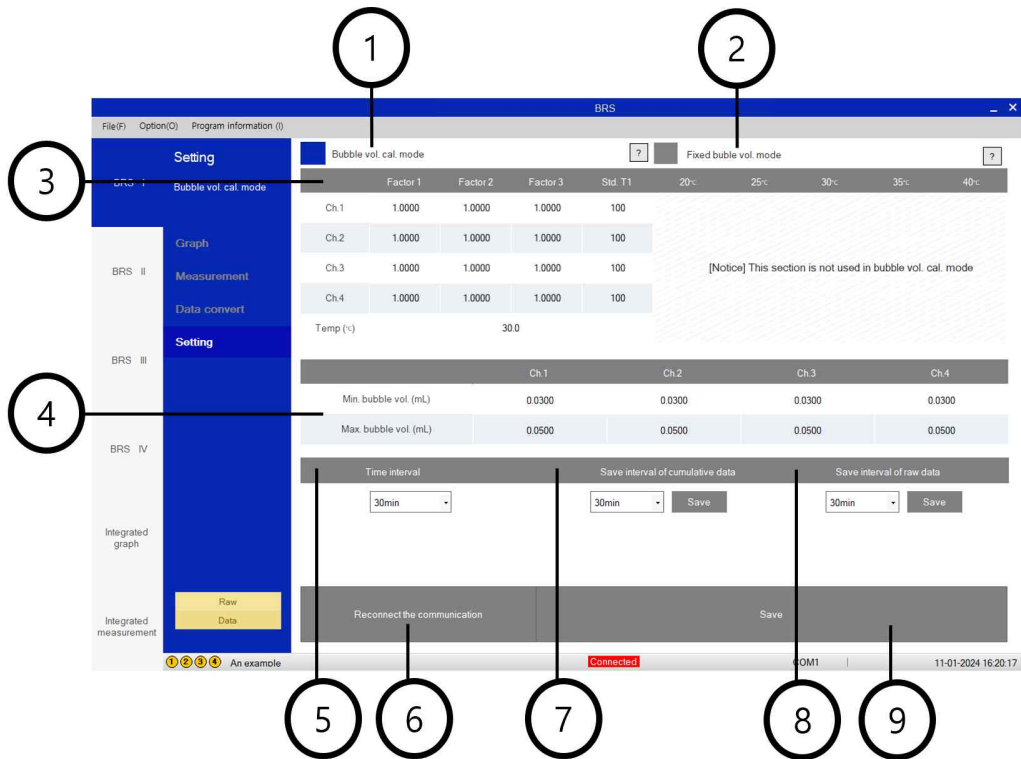


- ① Bubble vol. calc. mode
- ② Fixed bubble vol. mode
- ③ Input calibrating values for bubble vol. calc. mode
- ④ Min. and Max. bubble vol. (bubble vol. calc. mode only)
- ⑤ Time interval
- ⑥ Reconnect the communication
- ⑦ Save interval of cumulative data
- ⑧ Save interval of raw data
- ⑨ Save the setting

<Fixed bubble vol. mode>

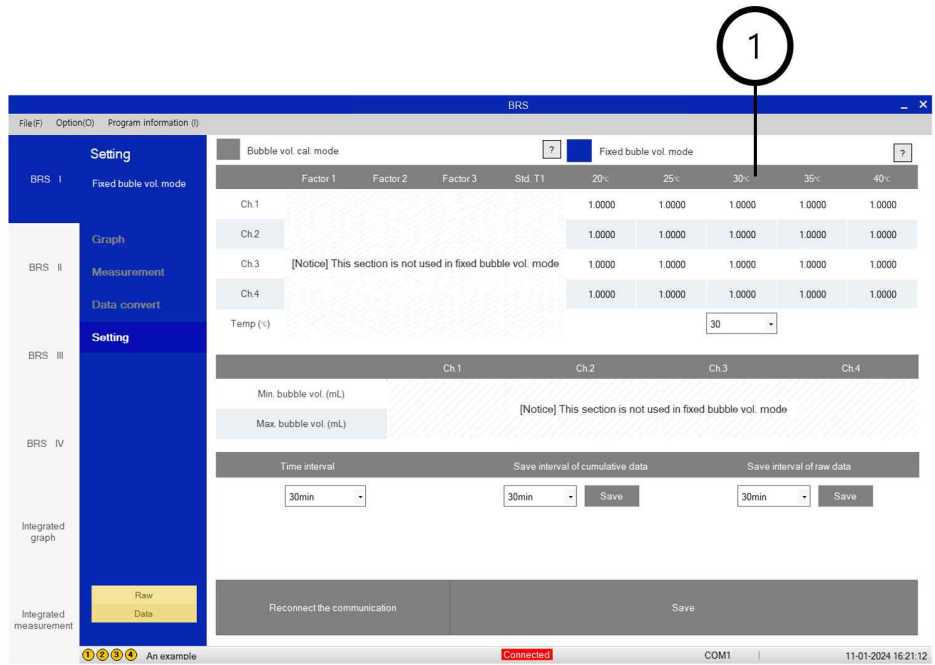


- ① Input bubble volumes at different temperatures in each cell in the fixed bubble vol. mode

(BRS-800)

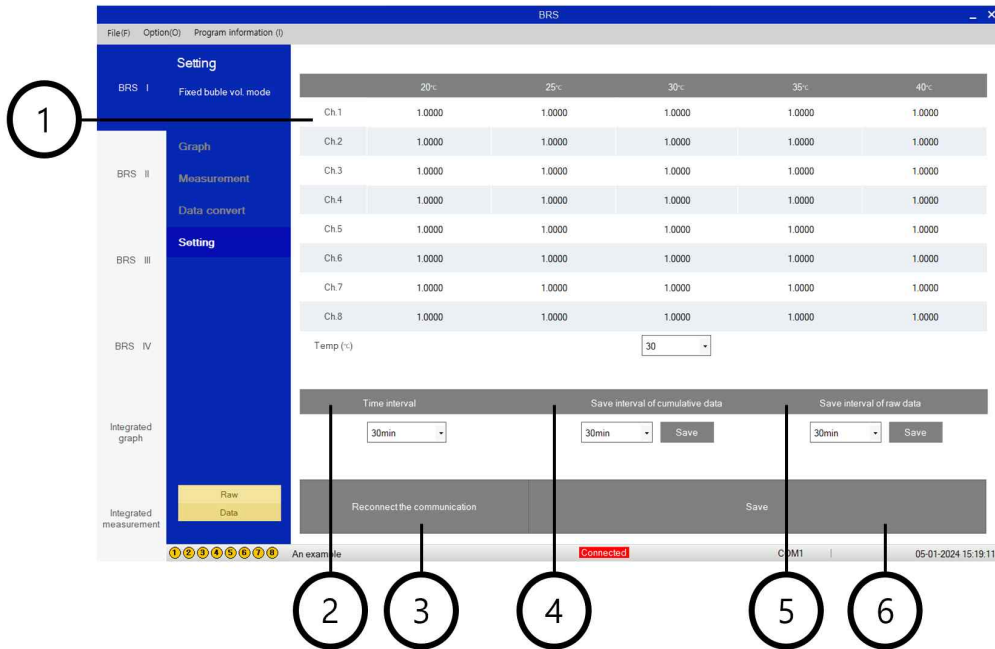


- ① Input calibrating values for fixed bubble vol. mode
- ② Time interval
- ③ Reconnect the communication
- ④ Save interval of cumulative data
- ⑤ Save interval of raw data
- ⑥ Save the setting

Integrated graph

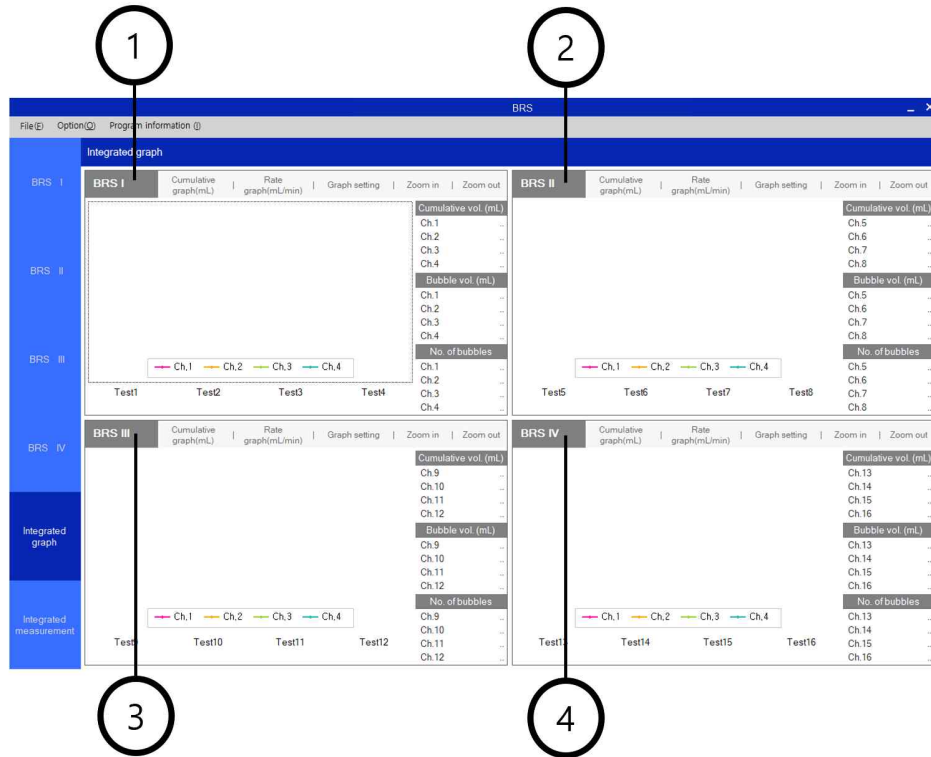


- ① BRS I graph
- ② BRS II graph
- ③ BRS III graph
- ④ BRS IV graph

④ Integrated measurement (BRS-110 and BRS-200)

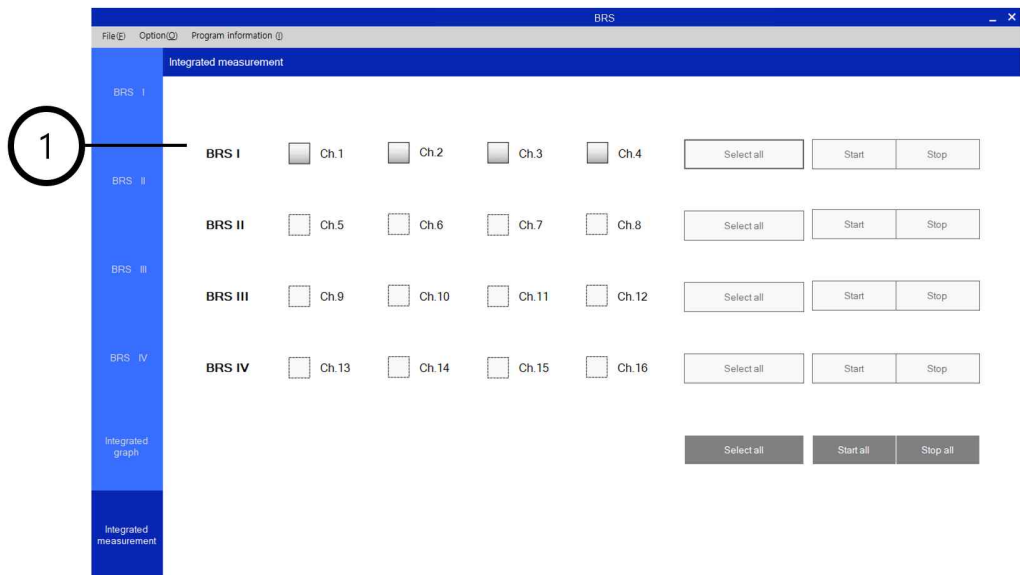

- ① Select the channels and start/stop measurement for the integrated measurement

(BRS-800)

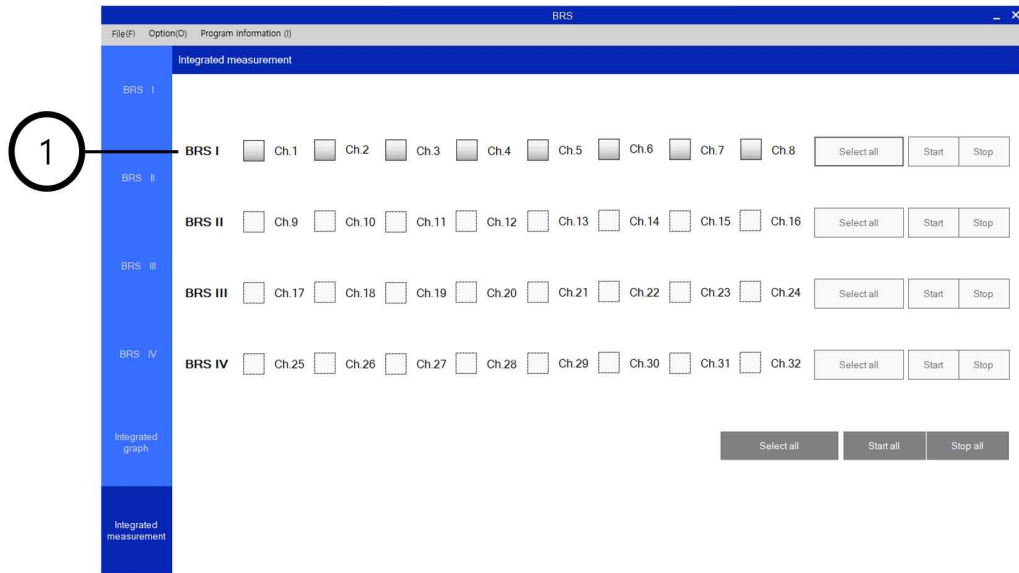

- ① Select the channels and start/stop measurement for the integrated measurement

Trouble shooting and maintenance

01

How to calibrate BRS cells for fixed bubble vol. mode

◉ Equipment preparation

- Syringe pump
- Gas tight syringe (10 mL)
- Incubator

◉ Calibration method

- ① Place the BRS device and a syringe pump in an incubator where the desired temperature is maintained, and leave them for more than 30 minutes to match the temperature of the oil in the BRS cell with the incubator temperature (as the temperature increases, the volume per bubble decreases)
- ② Connect the syringe in the syringe pump to the BRS cell of the device with tubing, and run the BRS program
- ③ Set the flow rate of the syringe pump at 2 mL/min, inject it for about 30 seconds, and check if bubbles are generated in the BRS cell
- ④ Change the flow rate of the syringe pump at 0.1 mL/min, and inject 8 mL (using a 10 mL gas tight syringe) to check the number of bubbles (repeat three times and use the average value. If there is a large variation in the number of bubbles, carefully repeat this step)
- ⑤ Calculate the volume per a bubble (the total volume of the injected volume/bubble numbers) and enter it into the program
- ⑥ Calibration is required for each BRS cell and must be entered into the program

02

Optic sensor adjustment

If a channel is not working or the red LED blinking of the optic sensor is not clear, the high and low optic sensors for the channel should be adjusted. Our respirometer device consists of a total of 4 channels, and two optic sensors are used for each channel (total of eight optic sensors). The optic sensor on the left side of each channel is for the high sensor; the optic sensor on the right side is for the low sensor (BRS-110 and BRS-200).

- When adjusting the optic sensor, use a flat-blade screwdriver and set the COARSE at MIN and set the FINE at 3 o'clock
- Add air to the BRS cell and make bubbles. If the red LED of the optic sensor is blinking, turn the FINE adjuster to the left or right and set it where the red LED blinks clearly.
- If the red LED is not blinking, turn the COARSE to the right and set it where the red LED blinks and turn the FINE to the left or right and set it where the red LED blinks clearly

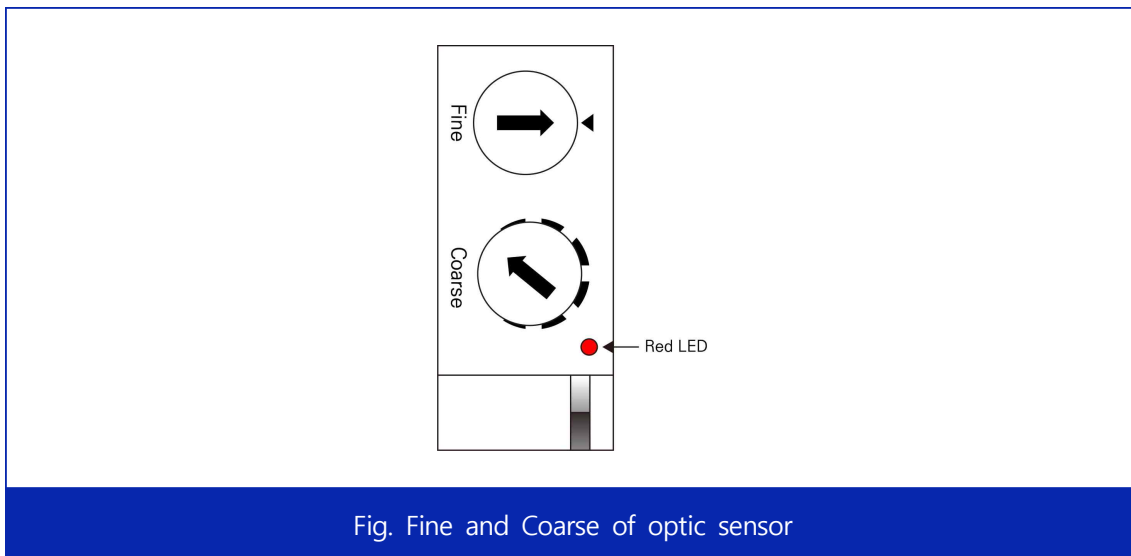


Fig. Fine and Coarse of optic sensor

How to adjust the optic sensor

	Adjustment methods	Coarse	Fine
Initial	Set the COASE adjuster at MIN and set the FINE adjuster at 3 o'clock		
If the LED is blinking	Turn the FINE adjuster to the left or right and set it where the red LED blinks clearly.	not need	
If the LED is not blinking	Turn the COARSE to the right and set it where the red LED blinks and turn the FINE to the left or right and set it where the red LED blinks clearly		

▶ When the graph is displayed in a step-like manner

- Due to blockages of needles, fittings, and tubing caused by water or small particles, the headspace pressure accumulates inside the bioreactor as gas produces over time, and when the blocked part is suddenly released due to pressure, a large amount of gas is released at once.
- If a water droplet forms at the tip of the needle inserted into the septum of the bioreactor, lightly tapping the needle with a finger can remove the water droplet.
- After separating needles, fittings, and tubing from the bioreactor, remove foreign substances by injecting air quickly using a syringe
- Replace any faulty needles, fittings, or tubings with new ones. If water droplets frequently form at the tip of a needle, consider using an alternative type of connection between the bioreactor and BRS cell

▶ If bubble generation is confirmed but the value is not displayed in the BRS program

- The power of the BRS device is not turned on or the USB is not properly connected
 - Check the power and USB connection of the BRS respirometer
- If the oil level in the measurement cell is not higher than the H.sensor when bubbles are generated
 - Remove the oil in the measurement cell, inject 2.2 mL (for BRS-110) or 12 mL (for BRS-200) or 1.6 mL (for BRS-800) of new oil
- Optic sensor adjustment is needed

▶ How to change oil in a BRS cell

When the BRS system is used, the oil in cells may be contaminated with water or particles from the outside. The oil should be changed.

- Slowly turn the right top fitting of the corresponding cell counterclockwise using a wrench and remove it.
- Remove the oil inside the cell with a disposable plastic dropper, etc., and then

use a cotton swab or a small piece of laboratory tissue to remove all remaining oil. To clean the cell, add some oil and do the same thing as described above. If possible, compressed air should then be injected into the cell to remove any remaining oil or unknown particles.

- After cleaning the cell, use a syringe to carefully inject right amount of BRS oil into the cell. Bubble generation should be checked by adding air into the cell using a syringe. If particles are present in the path in the BRS cell, the bubbles formed will be deflected, and the bubble size will be smaller.
- When everything is OK, join the disassembled fitting to the cell. After completing this oil change, it is necessary to calibrate the device. However, if the fixed bubble volume mode and the same amount of the same oil are used, recalibration should not be needed (BRS oil is a special oil made for the respirometer and can be purchased through the company).
- The characteristics of oils are different for BRS-110, BRS-200, and BRS-800).

04

Disabling power saving mode

 Disable power saving mode

- If power saving mode is enabled on the PC or laptop where BRS is installed, data communication may not be available




<For Windows 7>

[Control Panel] > [Power Options] > [Change when the computer sleeps]
- Change "Put the computer to sleep" to "Never"

<For Windows 10>

[Windows Settings] > [System] > [Power & sleep]
- Turn off the following options: "Sleep" and "Turn off the display"

05 Specifications

	BRS-110	BRS-200	BRS-800
			
No. of channels	4 (expandable 16 in a computer)	4 (expandable 16 in a computer)	8 (expandable 32 in a computer)
Flow rate	0~1 mL/min	1~5 mL/min	0~0.2 mL/min
Measuring resolution	Approx. 0.03 mL	Approx. 0.15 mL	Approx. 0.03 mL
Measuring interval	1 sec~10 hours(changeable)		
Gases	O ₂ (OUR), CO ₂ , CH ₄ , H ₂ , and N ₂		
Calibration error	≤1%		
Data output	USB		
Power input	DC 12V, 3.5A		
Weight	1.5 kg	1.9 kg	1.7 kg
Size	190(W)*130(D) *110*H), mm	200(W)*140(D) *120*H), mm	200(W)*140(D) *120*H), mm
Temperature	0~50℃		
Humiity	≤95%		
Material	Aluminum and acrylic		

User's manual v1.1

TEL +82-33-243-6449

FAX +82-33-242-6450

E-mail eetech2011@daum.net

WEB <http://www.eetech.co.kr>

A/S address Room 101, Building no. 309,
College of Agriculture and Life
Science, Kangwon National
University, Chuncheon-si, Gangwon
State, South Korea
Zip code : 24341

USER'S MANUAL

Biological Respirometric System (BRS)

- Biogas Respirometer / BMP Analyzer -

